



US009277829B2

(12) **United States Patent**  
**Jacofsky et al.**

(10) **Patent No.:** **US 9,277,829 B2**  
(45) **Date of Patent:** **Mar. 8, 2016**

(54) **SYSTEMS AND METHODS FOR MONITORING AND PROVIDING THERAPEUTIC SUPPORT FOR A USER**

USPC ..... 5/713, 615, 715, 710-712, 706;  
177/144  
See application file for complete search history.

(75) Inventors: **Marc C. Jacofsky**, Phoenix, AZ (US);  
**David J. Jacofsky**, Peoria, AZ (US)

(56) **References Cited**

(73) Assignee: **TC13—Pressure Applications LLC**,  
Phoenix, AZ (US)

U.S. PATENT DOCUMENTS

(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

4,542,547 A \* 9/1985 Sato ..... 5/713  
5,044,029 A 9/1991 Vrzalik  
(Continued)

(21) Appl. No.: **13/188,721**

FOREIGN PATENT DOCUMENTS

(22) Filed: **Jul. 22, 2011**

JP 2010-286971 A 12/2010

(65) **Prior Publication Data**

US 2013/0019408 A1 Jan. 24, 2013

OTHER PUBLICATIONS

European Search Report for EP 12817138.6, mailed May 4, 2015, 9 page.

(51) **Int. Cl.**  
**A47C 31/12** (2006.01)  
**A47C 27/08** (2006.01)  
**A61G 7/057** (2006.01)  
(Continued)

*Primary Examiner* — Robert G Santos  
*Assistant Examiner* — Myles Throop  
(74) *Attorney, Agent, or Firm* — Sterne, Kessler, Goldstein & Fox P.L.L.C.


(52) **U.S. Cl.**  
CPC ..... **A47C 31/123** (2013.01); **A47C 27/083** (2013.01); **A61B 5/447** (2013.01); **A61B 5/6832** (2013.01); **A61G 7/05776** (2013.01); **G06F 19/3406** (2013.01); **A61B 5/0022** (2013.01); **A61B 5/0024** (2013.01); **A61B 5/7275** (2013.01); **A61B 2562/028** (2013.01); **A61B 2562/0247** (2013.01); **A61G 2203/34** (2013.01); **A61G 2203/46** (2013.01); **A61G 2205/60** (2013.01)

(57) **ABSTRACT**


A method for monitoring pressure at one or more points on an individual and automatically adjusting one or more sections of a support structure. The method includes periodically receiving pressure data from one or more radio frequency addressable sensors placed on an individual; determining, based on the received pressure data, whether an adjustment in the support structure is required; systematically adjusting cells located within the plurality of zones, one zone at a time, until an improvement in pressure data is indicated. If an improvement in pressure data is indicated for a zone, systematically adjusting cells within the plurality of subzones for that zone, one subzone at a time, until an improvement in pressure data is indicated. If an improvement in pressure data is indicated for a subzone, systematically adjusting cells in that subzone, one cell at a time, until an improvement in pressure data is indicated.

(58) **Field of Classification Search**  
CPC ..... A61G 7/05769; A61G 2203/34; A61G 7/05776; A61G 2203/46; A61G 2205/60; A61G 2203/03; A47C 27/082; A47C 27/10; A47C 27/083; A47C 31/123; A61B 5/447; A61B 5/6832; A61B 5/0022; A61B 2562/028; A61B 2562/0247; A61B 5/7275; A61B 5/0024; G06F 19/3406

**25 Claims, 16 Drawing Sheets**

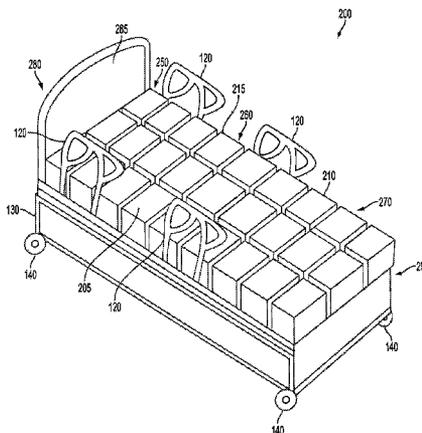

(51)	<p><b>Int. Cl.</b>  <i>G06F 19/00</i> (2011.01)  <i>A61B 5/00</i> (2006.01)</p>	<p>7,786,874 B2 * 8/2010 Rodgers ..... 340/573.1  7,789,086 B2 * 9/2010 Hyde et al. .... 128/845  7,802,332 B2 9/2010 Kummer et al.  7,849,544 B2 12/2010 Flocard et al.  7,849,545 B2 12/2010 Flocard et al.  RE43,532 E * 7/2012 Menkedick et al. .... 5/618  8,306,666 B2 * 11/2012 Huber et al. .... 700/275  2006/0065060 A1 3/2006 Ito et al.  2006/0179579 A1 8/2006 Phillips et al.  2007/0199154 A1 8/2007 Escaross  2008/0091092 A1 * 4/2008 Al-Ali ..... 600/310  2008/0201847 A1 8/2008 Menkedick et al.  2009/0088608 A1 * 4/2009 Mumford et al. .... 600/300  2010/0109848 A1 5/2010 Blair et al.  2010/0298742 A1 * 11/2010 Perlman et al. .... 600/595  2011/0004276 A1 1/2011 Blair et al.  2012/0003933 A1 * 1/2012 Baker et al. .... 455/41.2  2012/0010525 A1 * 1/2012 Jacofsky et al. .... 600/561  2013/0006151 A1 * 1/2013 Main et al. .... 600/587  2013/0340176 A1 * 12/2013 Stevens et al. .... 5/710</p>
(56)	<p style="text-align: center;"><b>References Cited</b></p> <p style="text-align: center;">U.S. PATENT DOCUMENTS</p> <p>6,145,143 A 11/2000 Hicks et al.  6,216,300 B1 4/2001 Hannagan  6,421,859 B1 7/2002 Hicks et al.  6,463,336 B1 * 10/2002 Mawhinney ..... 607/156  6,560,804 B2 * 5/2003 Wise et al. .... 5/713  6,591,437 B1 7/2003 Phillips  6,874,185 B1 4/2005 Phillips et al.  6,892,405 B1 * 5/2005 Dimitriu et al. .... 5/615  7,225,488 B2 6/2007 Wu  7,444,704 B2 * 11/2008 Phillips et al. .... 5/713  7,583,199 B2 9/2009 Graebe, Jr.  7,685,662 B2 3/2010 Viard  7,784,131 B2 8/2010 Genaro et al.</p>	<p>* cited by examiner</p>

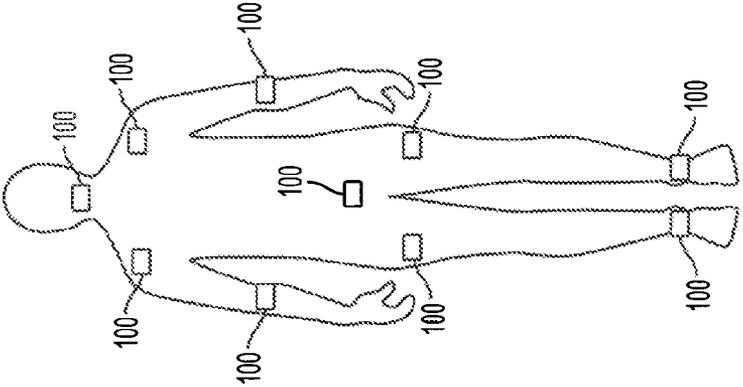

PATIENT - REAR VIEW

FIG. 1B

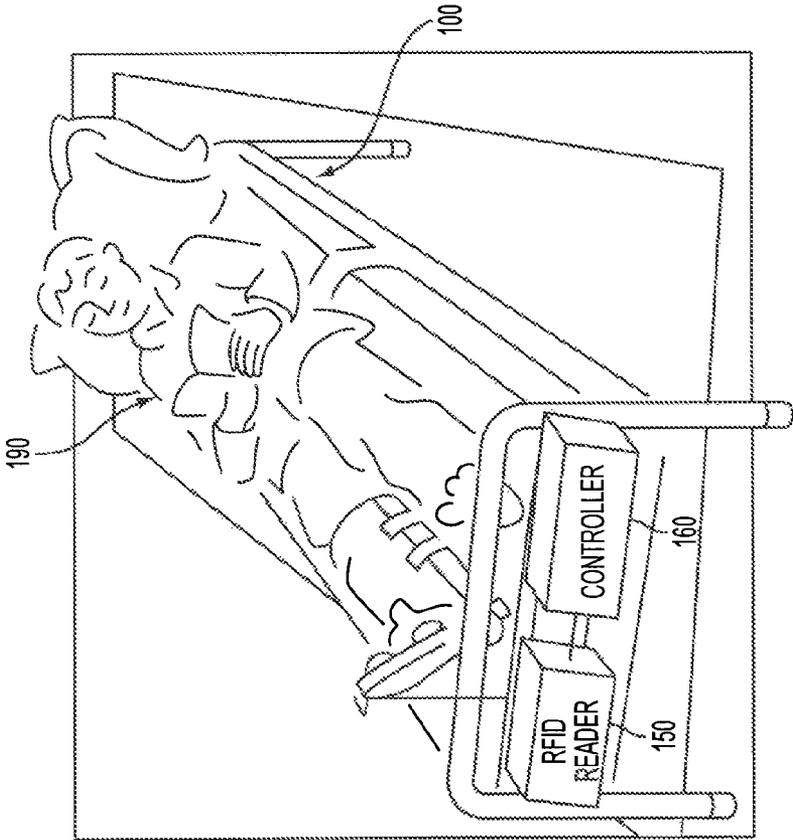


FIG. 1A

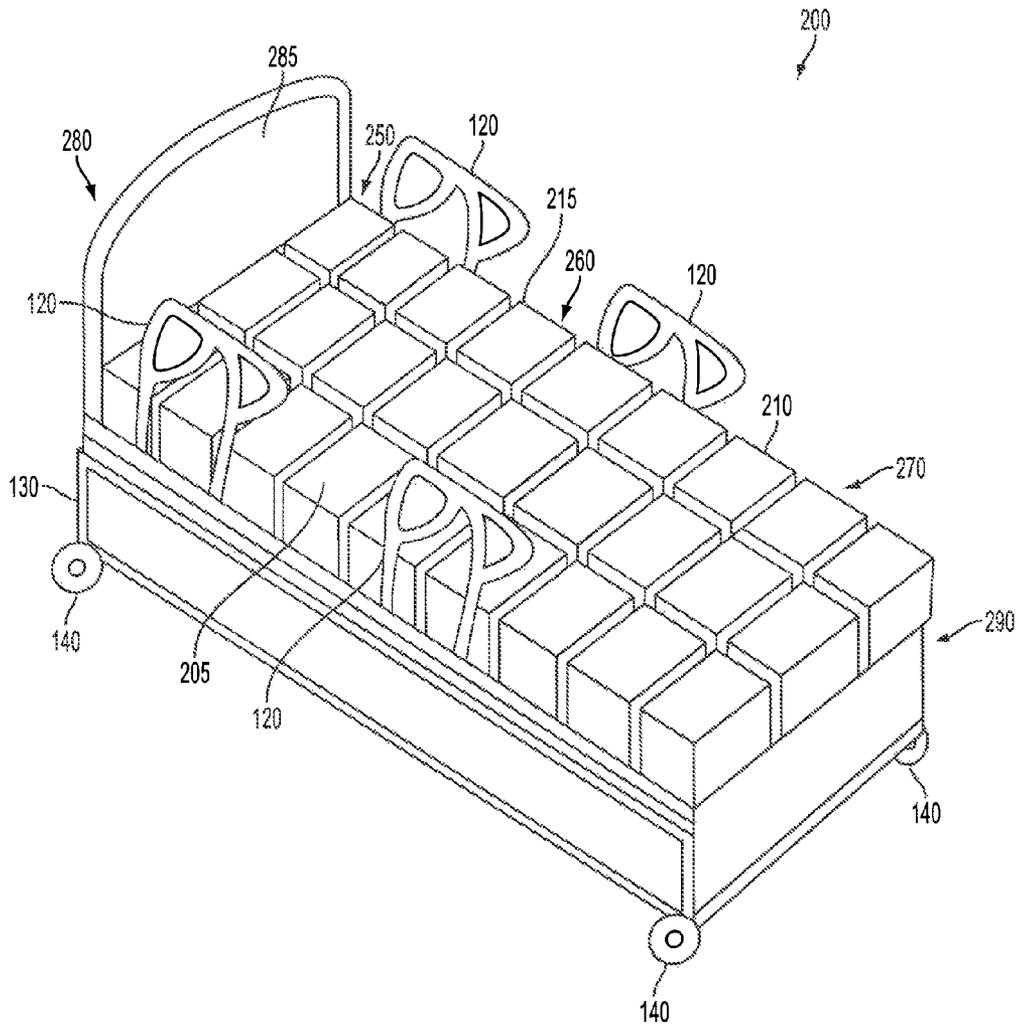


FIG. 2

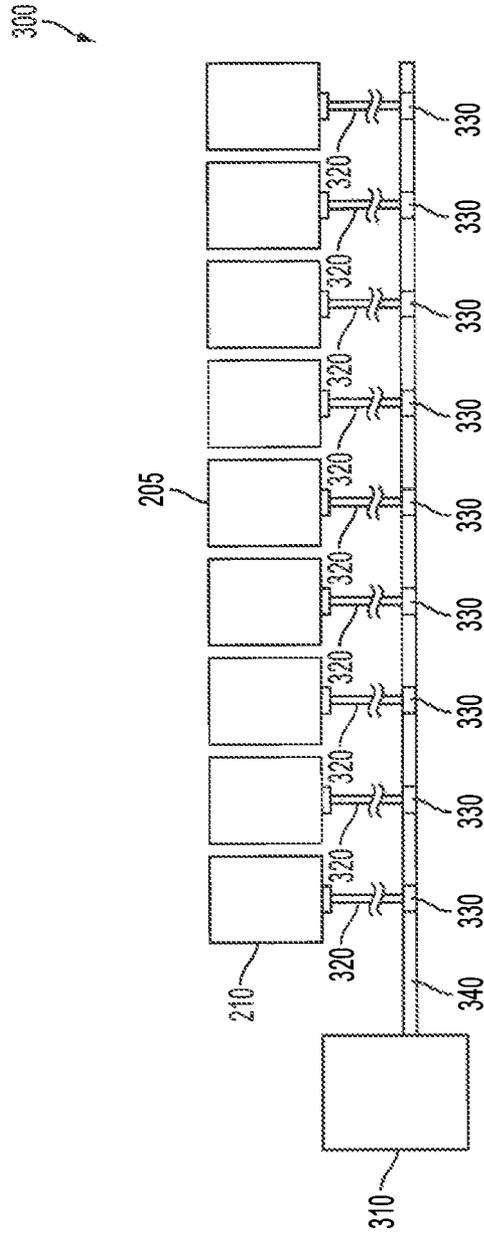


FIG. 3

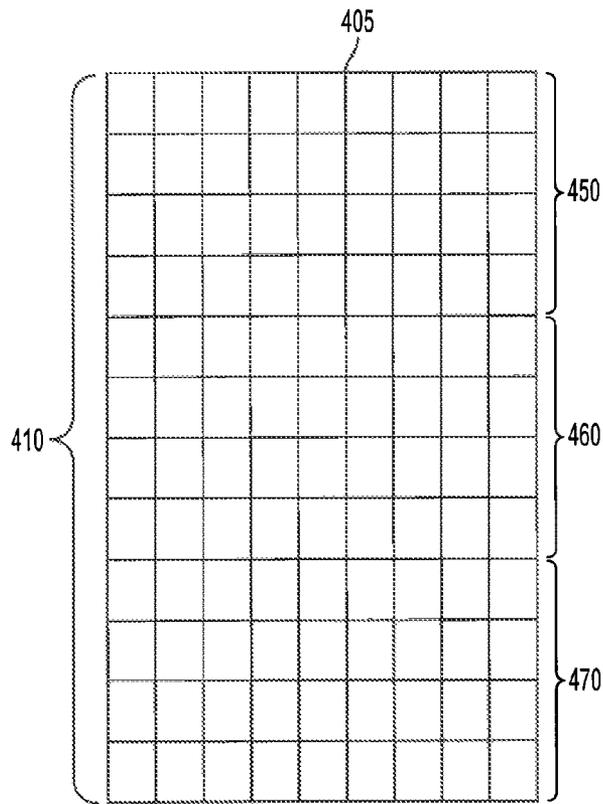


FIG. 4

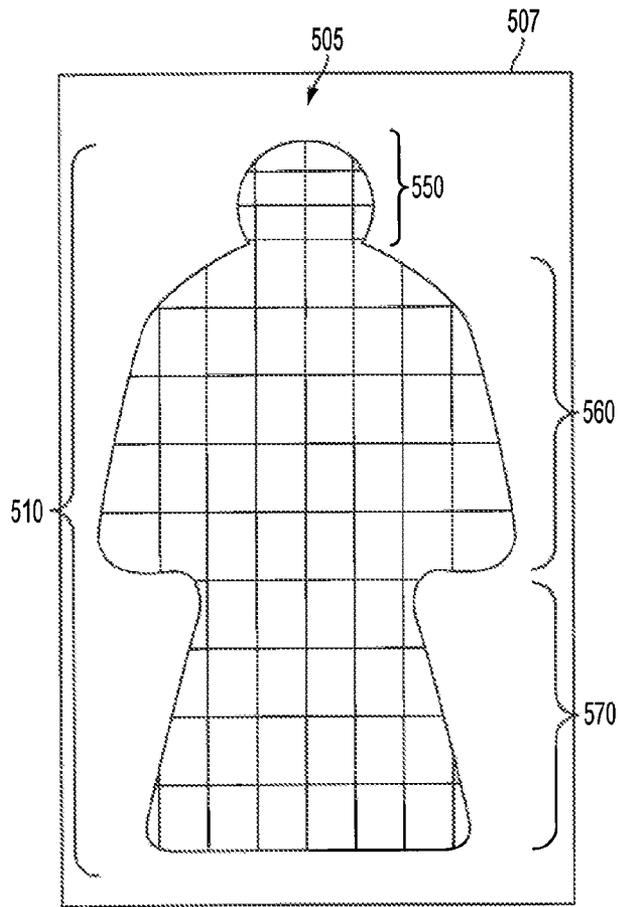


FIG. 5

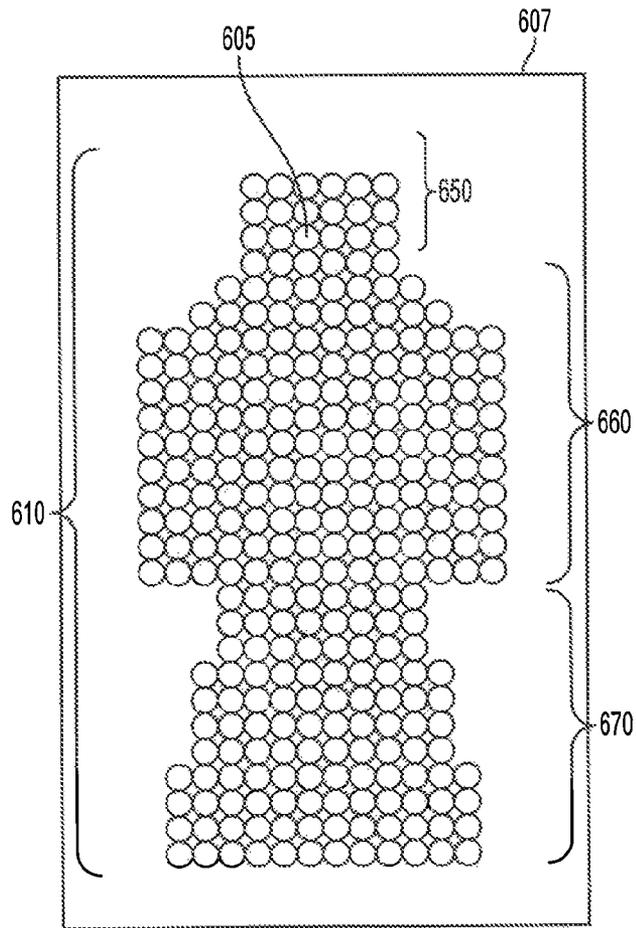


FIG. 6

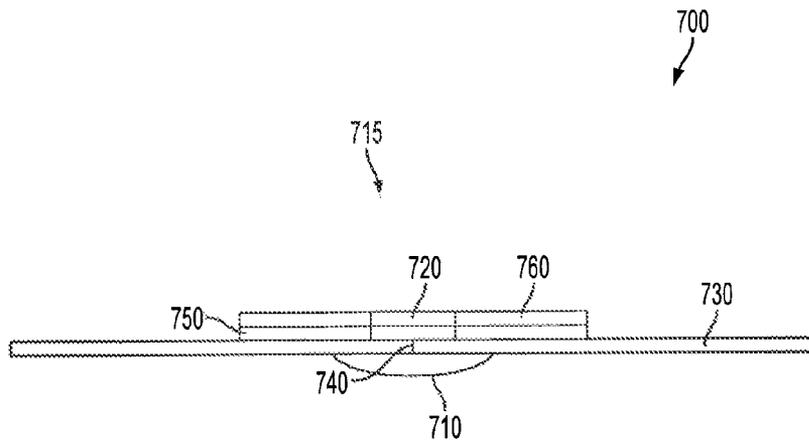


FIG. 7

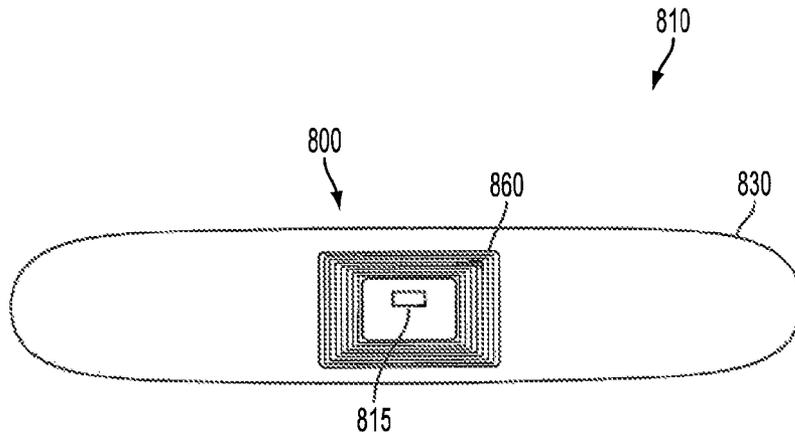


FIG. 8

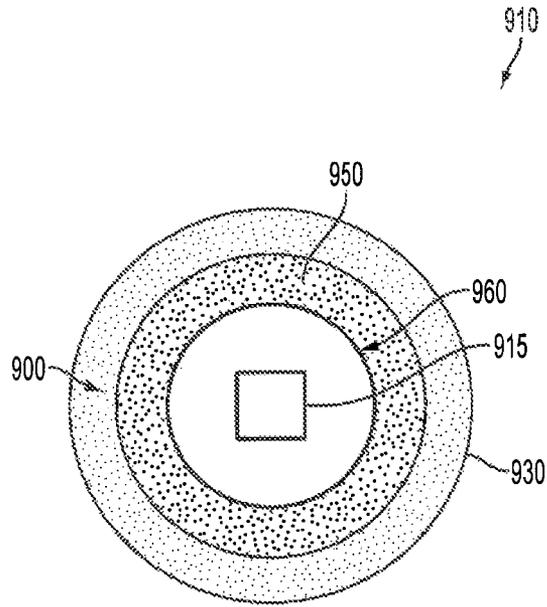


FIG. 9

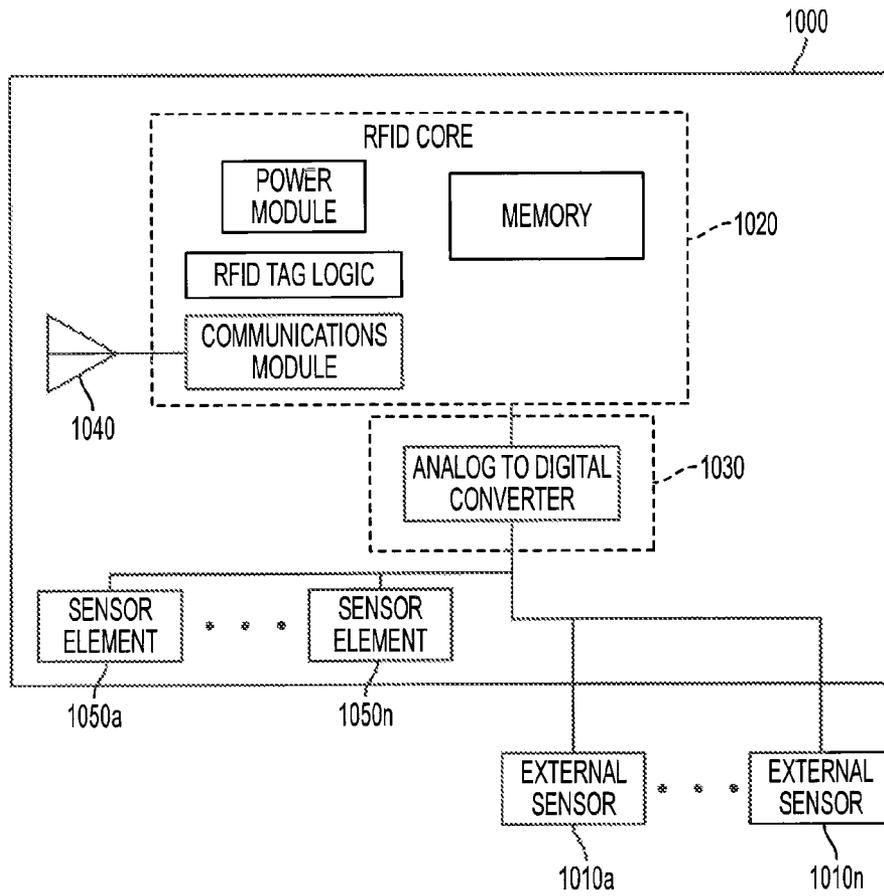


FIG. 10

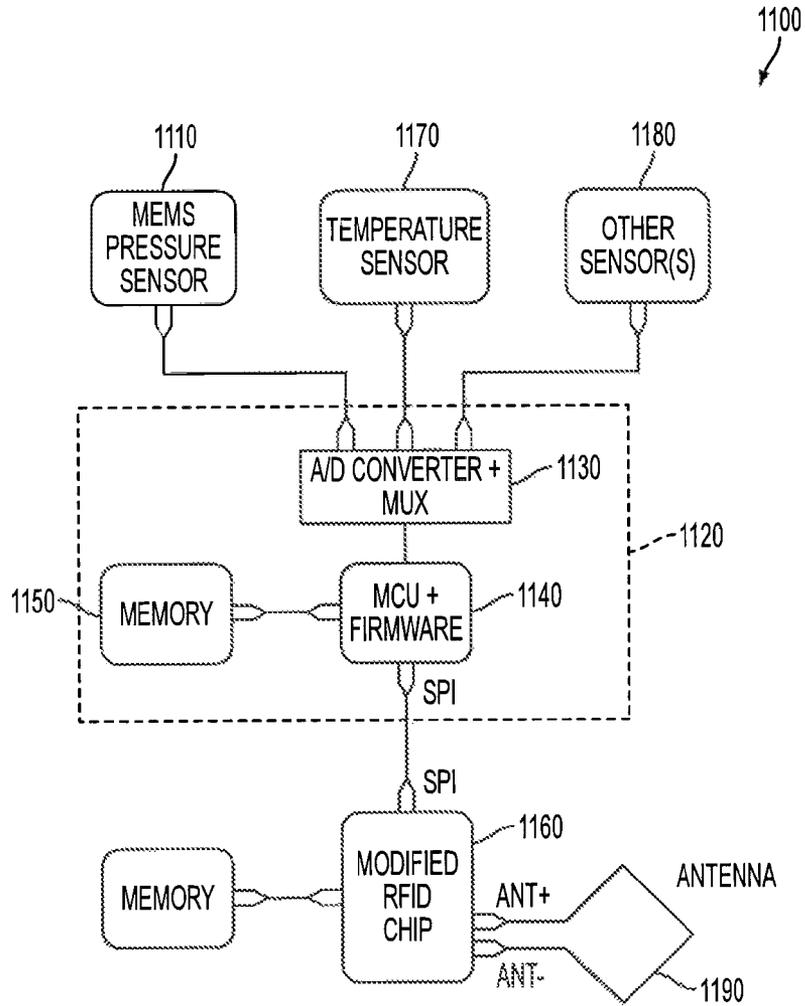


FIG. 11

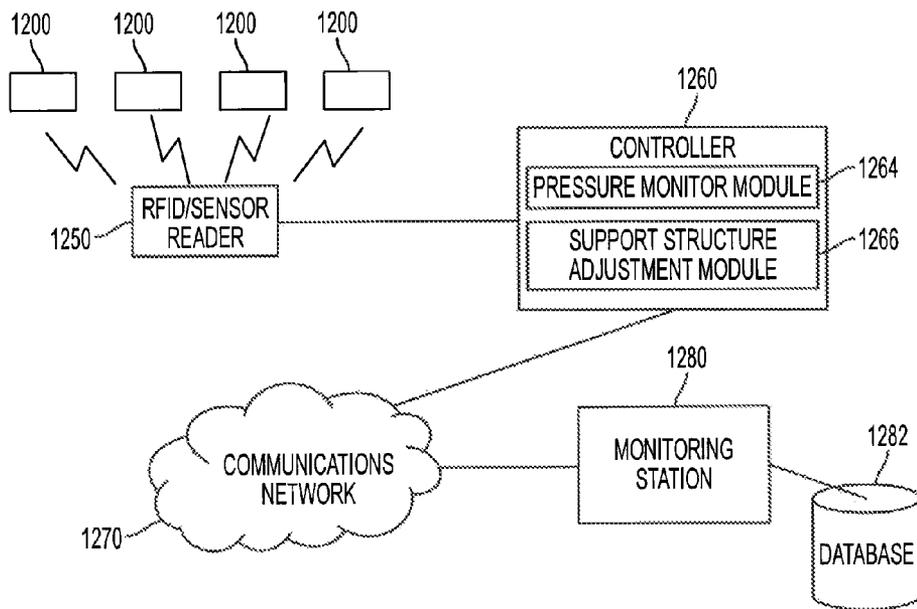


FIG. 12

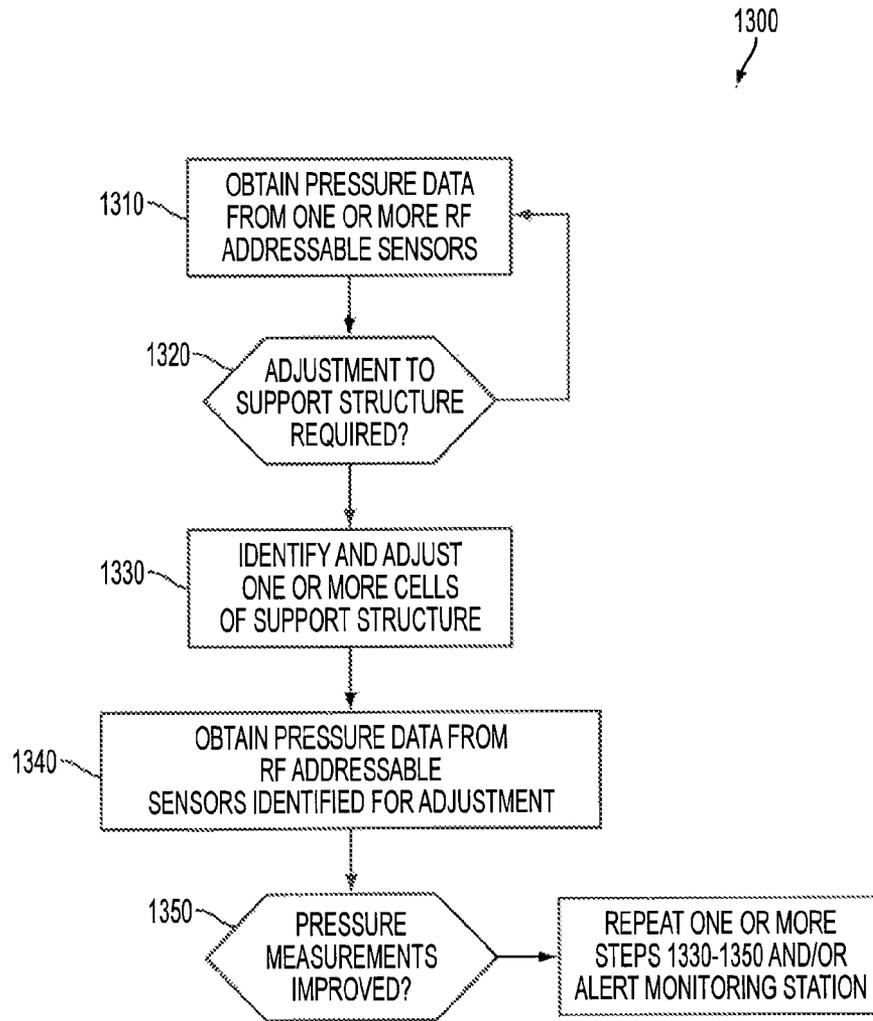


FIG. 13

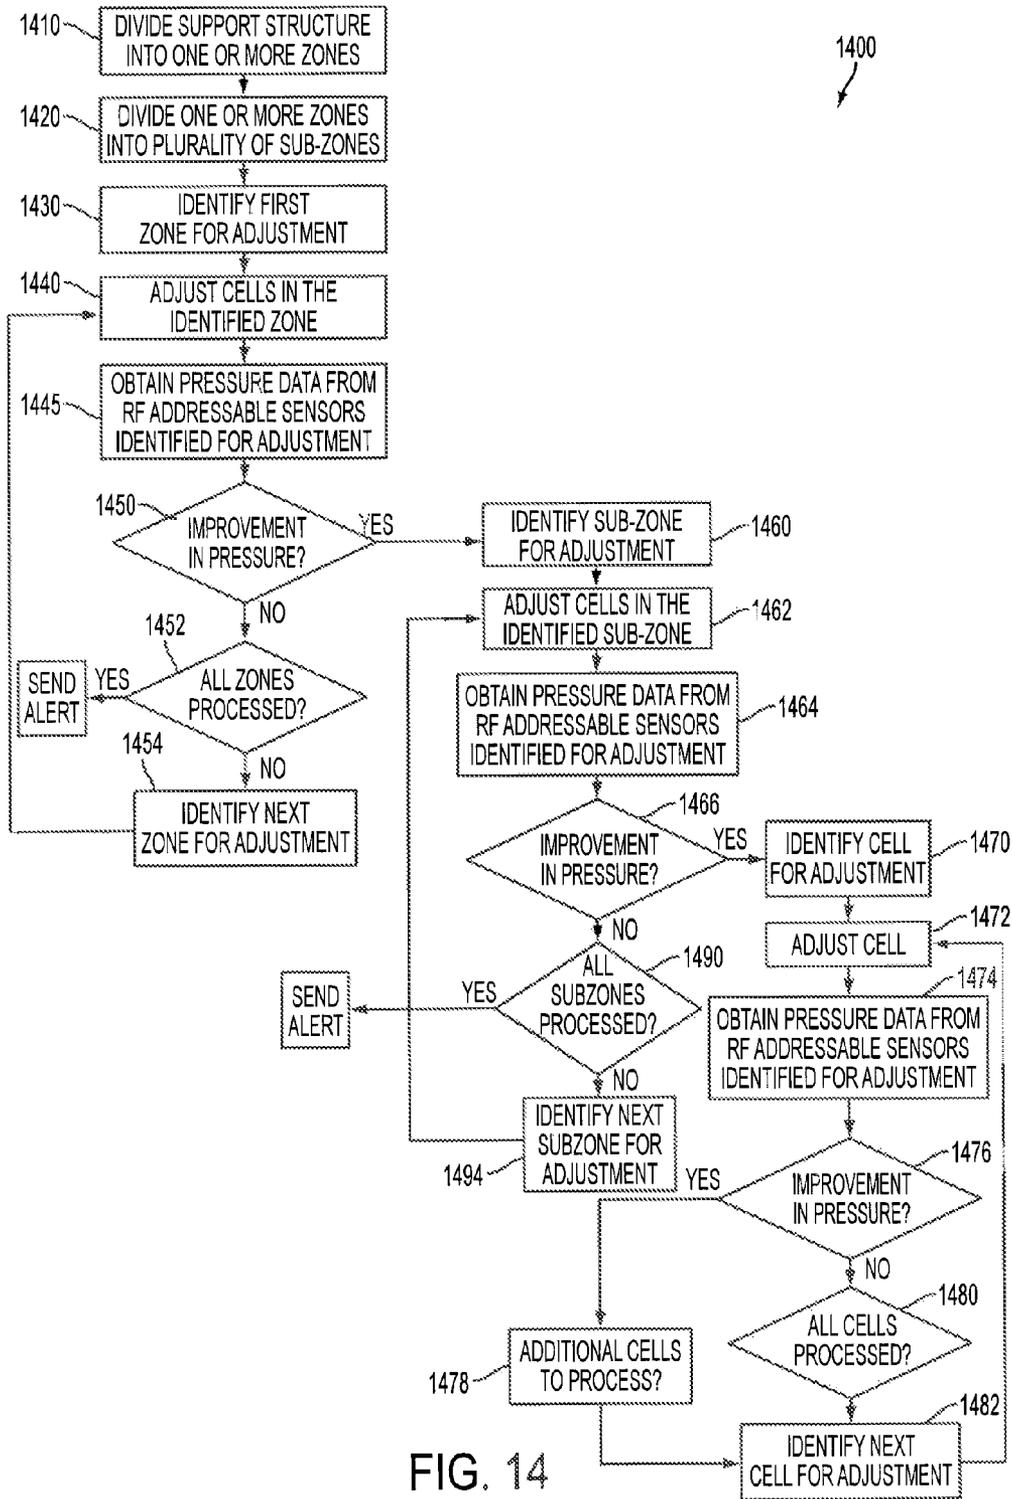


FIG. 14

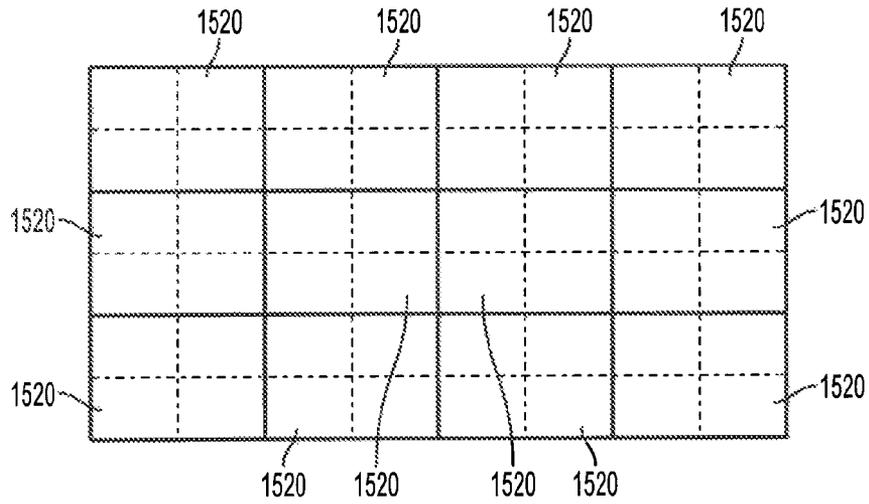


FIG. 15A

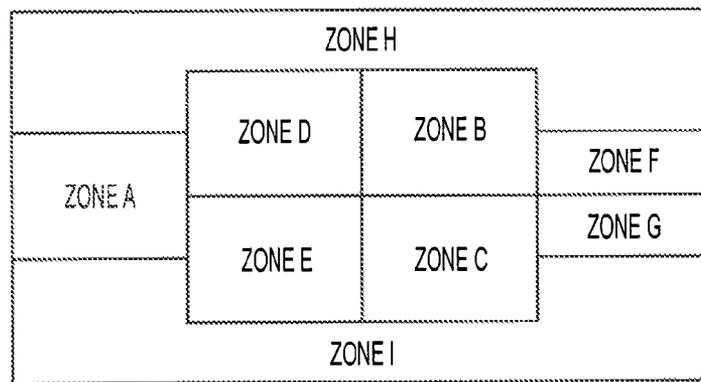


FIG. 15B

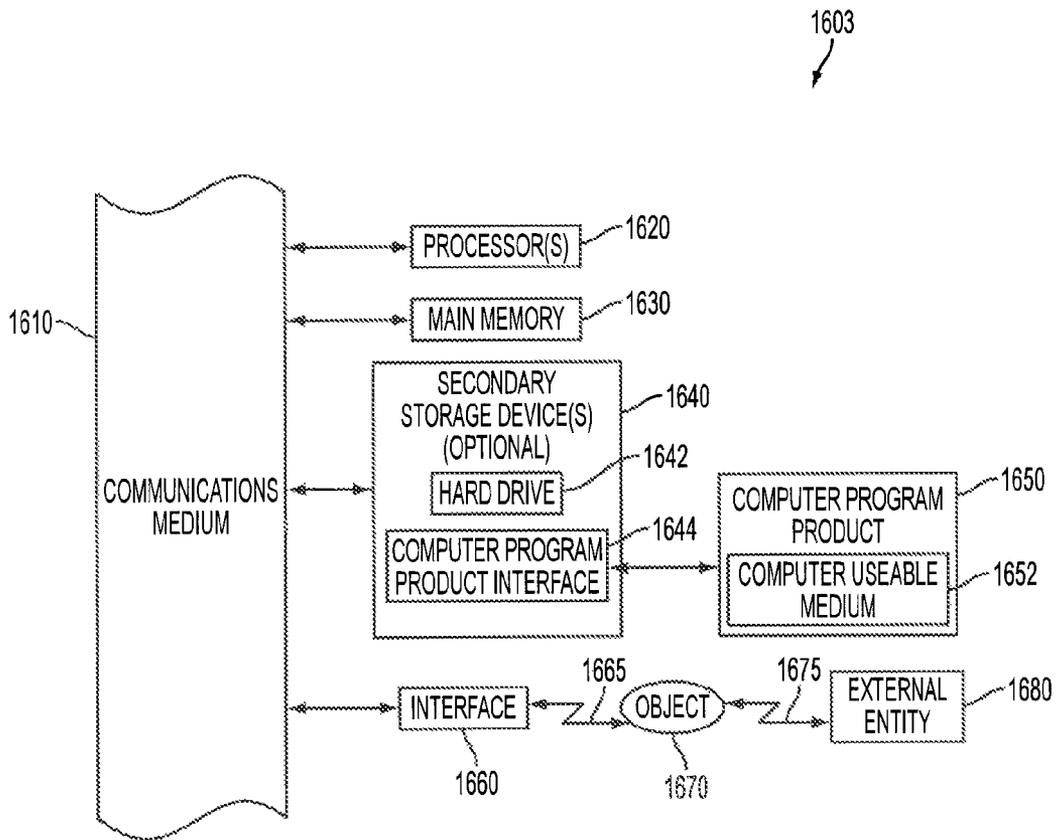


FIG. 16

# SYSTEMS AND METHODS FOR MONITORING AND PROVIDING THERAPEUTIC SUPPORT FOR A USER

## FIELD OF THE INVENTION

The present invention is related to systems and methods for monitoring pressure exerted on an individual at one or more points by a support structure and adjusting the support structure, in response to the monitored pressure.

## BACKGROUND

The prevention and treatment of bedsores (and similar pressure injuries) is a serious issue facing hospitals and other healthcare facilities. Bedsores (also known as decubitus ulcers or pressure sores) result from prolonged pressure on an area. For example, a bedsore is a tissue injury that develops when soft tissue is compressed between a bony prominence and an external surface for a prolonged period of time. Bedsores are most likely to form on the back of the head, the sacrum, heels, ankles, buttocks, or shoulders. Bedsores are painful and can be life-threatening to patients, particularly the elderly and disabled. Excessive pressure on recent surgical incisions can lead to wound healing complications with similar etiology. The National Decubitus Foundation estimated that as many as 16% of the population of U.S. hospitals, alone, suffered from some form of pressure wound such as a bedsore.

Bedsores are most common for patients confined to a bed, chair or wheelchair. These furniture support systems often include padding made from cotton, feathers, foam, or the like. Some techniques for preventing bedsores focus on the design of the furniture and padding. To ease pressure, furniture has been introduced that include a fixed quantity of air or liquid in one or more chambers to provide therapeutic benefits, including minimizing the severity of pressure points on a user's body. In addition, some of these support systems include manual or programmable adjustable cushion sections. However, these systems cannot be adjusted based on feedback about the current condition of a patient and therefore, a patient may still develop bedsores using therapeutic furniture. Once a bedsore develops it is important to mitigate continued excessive pressure to the region to facilitate the healing process.

Another typical method for preventing bedsores involves frequent repositioning of a patient. However, this method of prevention is highly time consuming for medical and care facilities, particularly facilities having a large number of disabled or immobile patients. What is therefore needed is a system that can automatically adjust a support structure (or external padding for furniture) based on pressure monitored on one or more areas of a patient.

## BRIEF DESCRIPTION OF THE FIGURES

The accompanying drawings, which are incorporated herein, form part of the specification and illustrate embodiments of systems and methods for monitoring and providing therapeutic support for a user. Together with the description, the drawings further serve to explain the principles of, and to enable a person skilled in the relevant art(s) to make and use the systems and methods described herein. In the drawings, like reference numbers indicate identical or functionally similar elements.

FIGS. 1A and B illustrate an exemplary operating environment for a system for monitoring pressure for an individual

confined for a period of time to a support structure, such as a bed or a chair, according to embodiments of the present invention.

FIG. 2 is a perspective view of a support system incorporating a system for monitoring and providing therapeutic support for a user, in accordance with an embodiment of the present invention.

FIG. 3 is a schematic view of an air hose assembly of the support system of FIG. 2 in accordance with an embodiment of the present invention.

FIG. 4 is a schematic view of a support surface in accordance with an embodiment of the present invention.

FIG. 5 is a schematic view of a support surface in accordance with an embodiment of the present invention.

FIG. 6 is a schematic view of a support surface in accordance with an embodiment of the present invention.

FIG. 7 is a schematic view of a pressure monitor in accordance with an embodiment of the present invention.

FIG. 8 is a top view of a bandage incorporating a pressure monitor in accordance with an embodiment of the present invention.

FIG. 9 is a top view of an alternate embodiment of a bandage incorporating a monitor in accordance with an embodiment of the present invention.

FIG. 10 is an RF device in accordance with an embodiment of the present invention.

FIG. 11 depicts an exemplary system having a modified RFID chip, in accordance with an embodiment.

FIG. 12 is a block diagram of an illustrative network for remotely monitoring one or more sensors integrated with RF devices, in accordance with an embodiment of the present invention.

FIG. 13 is a flowchart illustrating a method of monitoring pressure, in accordance with an embodiment.

FIG. 14 is a flowchart showing a method for linking identifiers to create transparent and secure wireless monitoring of a user, in accordance with an embodiment.

FIG. 15A depicts an exemplary support structure.

FIG. 15B depicts an exemplary support structure.

FIG. 16 illustrates a block diagram of a data processing unit that can be used to implement portions of the RFID reader/sensor or controller illustrated in FIG. 12.

## DETAILED DESCRIPTION

The following detailed description of systems and methods for monitoring and providing therapeutic support for a user refers to the accompanying drawings that illustrate exemplary embodiments. Unless otherwise noted, all embodiments and examples should be considered prophetic examples. Other embodiments are possible. Modifications can be made to the embodiments described herein without departing from the spirit and scope of the present invention. Therefore, the following detailed description is not meant to be limiting. Further, it would be apparent to one of skill in the art that the systems and methods described below can be implemented in many different embodiments of hardware, software, and/or firmware. Any actual hardware, software, and/or firmware described are not meant to be limiting.

Presented herein are embodiments of systems and methods for monitoring pressure on a patient and adjusting a support structure accordingly. In one embodiment, a pressure monitor can continuously (or semi-continuously) measure contact pressures between a portion of a user's body and a section of a support surface of a support system, such as a hospital bed. For example, the pressure monitor can measure contact pres-

sure between a support surface and the user's head, arms, legs, feet, arms, torso, or any other suitable location on the user.

In embodiments, a pressure monitor can be configured to transmit measured pressure data to a networkable device (e.g., a laptop computer, PDA, cell phone, a processor located in the bed, or other patient monitor) using RF communications. The networkable device can then send a signal to actuators located within the bed to adjust the pressure of one or more sections in the support surface of the bed. The networkable device can additionally communicate the user's status and condition to a healthcare provider station (e.g., staffed by nurses, doctors, and other hospital personnel) or directly to a healthcare providers' wireless networkable device (e.g. cell phone, pager, or personal digital assistant (PDA)) through a communication network such as a local area network (LAN), wide area network (WAN), or the like. This communication allows the healthcare provider to remotely monitor a user, such as a hospital patient and take action when certain conditions are indicated. The networkable device, or associated computing system, can additionally record and display temporal trends, minima, and maxima in the pressure data and optionally log the data to the patient's electronic health records. The networkable device, or associated computing system, can also compare the pressure data to the patient's diastolic blood pressure or other measurement, and calculate relevant clinical gradients in real time.

FIGS. 1A and B illustrate an exemplary operating environment for a system for monitoring pressure for an individual confined to a support structure for a period of time, such as a bed or a chair, according to an embodiment of the present invention. As shown in FIG. 1A, the system includes a support system 110. In the example of FIG. 1A, the support system is depicted as a bed. However, as discussed in detail below, the support system may be a mattress pad, a chair such as wheelchair or a similar form of support. An individual, e.g., patient 190, comes into direct or indirect contact with the support system. As shown in FIG. 1A, the individual is lying on structure 110. However, in other embodiments, the individual may be sitting or reclining in a different position.

Prior to placement on the support structure, one or more RF addressable pressure sensors 100 are placed on the individual. These pressure sensors may be placed at locations highly susceptible to pressure injuries such as the sacrum, back of the head, elbows, shoulders, ankles, etc. In an embodiment, these sensors are placed on the skin of the patient in a location most likely to have direct or indirect contact with the support structure or upon which the support structure is likely to exert pressure. FIG. 1B is the rear view of a patient depicting exemplary placement of a plurality of RF addressable pressure sensors, according to embodiments of the present invention. RF addressable pressure sensors 100 are described in further detail below.

The system further includes an RFID reader 150 and a controller 160. Although depicted as separate components, RFID reader 150 and controller 160 could be implemented in a single structure. RFID reader 150 is configured to communicate with the one or more RF addressable pressure sensors 100 and obtain data therefrom. RFID reader 150 is placed proximate to the individual. Although FIG. 1A depicts the reader 150 attached to the foot of the bed, the RFID reader may be placed at any location to permit detection and access to the RF addressable sensors. For example, RFID reader 150 may be placed on the support structure, under the support structure, above the support structure, or next to the support structure (e.g., on a mobile station).

RFID reader 150 is coupled to a controller 160. In an embodiment, controller 160 is configured to receive data from reader 150 and to determine whether adjustments should be made to support structure to reduce pressure in one or more areas. In an alternative embodiment, reader 150 includes the logic to determine whether adjustments should be made to support structure. Controller 160 is further configured to cause adjustments to be made to the support structure.

In addition, RFID reader 150 and/or controller 160 may be connected to an external monitoring station. The communication infrastructure is described in further detail below.

### Support Systems

FIG. 2 is a perspective view of a support system 200 incorporating a system for monitoring and providing therapeutic support for a user, in accordance with an embodiment of the present invention. Support system 200 can be one of many forms, including but not limited to, a bed including a mattress and bed frame, such as a hospital bed configured for use during or after medical procedures, a conventional bed used for sleeping, a mattress for a bed, a mattress cover configured to be placed on top of a mattress, a chair such as a wheelchair, couch, or any other suitable support system having a support surface.

In some embodiments, support system 200 comprises conventional components of a hospital bed, for example mattress 215, head end 280 on one side of the mattress, including headboard 285, foot end 290 on the opposite side of mattress 215, bed frame 130 disposed underneath and supporting mattress 215, and side rails 120 for constraining a user within support system 200. Support system 200 can further include wheels 140 to facilitate moving the system. Alternatively, the support system can be in the form of a padded layer to be placed on top of a mattress, chair, couch, or other surface.

In some embodiments, mattress 215 can include a support surface 205 which includes areas corresponding to a conventionally sized user's body. For example, head portion 250 can be configured to receive the user's head, torso portion 260 can be configured to receive the user's torso, and leg portion 270 can be configured to receive the user's legs and feet. Mattress 215 can further include a plurality of adjustable sections 210. In some embodiments, each of adjustable sections 210 are in the shape of a square and are arranged to form a square grid, in other embodiments, one or more of adjustable sections 210 can be in the form of a shape other than a square. For example, a non-square rectangle, an oval, a sphere, a cylinder, or any other suitable geometric shape. In some embodiments, one or more sections can be shaped to contour the shape of the user's body. For example, mattress 215 can include a single adjustable section or a plurality of adjacent adjustable sections formed to provide a recess contour for the user's head.

In some embodiments, adjustable sections 210 of mattress 215 include a confined gas, liquid or other suitable flowable material. The support characteristics, such as inflation level can be adjusted with the aid of an air or liquid supply means, such as one or more pumps or a centralized facility air supply. In some embodiments, a single pump provides air to each of the sections. In other embodiments, multiple pumps provide air to multiple sections.

FIG. 3 is a schematic view of air hose assembly 300 of the support system of FIG. 2. In some embodiments, adjustable sections 210 are operatively connected to air pump assembly 310 to allow for inflation and deflation of adjustable sections 210. For example, air hose assembly 300 can be attached to central air line 340, which is then delivered through branch air

5

lines 320 via line connections 330. Branch air lines 320 are also operatively connected to adjustable sections 210 to provide for inflation and deflation. Line connections 330 may include individual solenoid valves or other means of controlling flow into or out of each chamber.

FIG. 4 is a schematic view of a support surface 405 in accordance with an embodiment. Like support surface 205 of FIG. 2, support surface 405 comprises portions corresponding to a conventionally sized user's body. For example, head portion 450 can be configured to receive the user's head, torso portion 460 can be configured to receive the user's torso, and leg portion 470 can be configured to receive the user's legs and feet. Adjustable sections 410 can be smaller in size compared to adjustable sections 210 of support surface 205 shown in FIG. 2. Adjustable sections 210 can be of any suitable size and shape.

FIG. 5 is a schematic view of a support surface 505 in accordance with an embodiment. Like support surface 205 of FIG. 2, support surface 505 comprises portions corresponding to a conventionally sized user's body. For example, head portion 550 can be configured to receive the user's head, torso portion 560 can be configured to receive the user's torso, and leg portion 570 can be configured to receive the user's legs and feet. Adjustable sections 510 can be arranged to generally follow the outline of the user's body in various conventional positions, as shown for Example in FIG. 2. In some embodiments, support surface 505 can further comprise an outer section 507 that surrounds the adjustable sections. Outer section 507 can comprise conventional bedding materials, such as foam or other padding, can alternatively comprise additional adjustable sections, non-adjustable inflated sections, or any suitable combination thereof.

FIG. 6 is a schematic view of a support surface 605 in accordance with an embodiment. Like support surface 205 of FIG. 2, support surface 605 comprises portions corresponding to a conventionally sized user's body. For example, head portion 650 can be configured to receive the user's head, torso portion 660 can be configured to receive the user's torso, and leg portion 670 can be configured to receive the user's leg and feet. Adjustable sections 610 can be arranged to generally follow the outline of the user's body in various conventional positions, as shown, for example, in FIG. 2. In some embodiments, support surface 605 can further comprise an outer section 607 that surrounds the adjustable sections. Outer section 607 can comprise conventional bedding materials, such as foam or other padding, can alternatively comprise additional adjustable sections, non-adjustable inflated sections, or any suitable combination thereof. Adjustable sections 610 can be rectangular in shape and smaller in size compared to adjustable sections 210 shown in FIG. 2 and adjustable sections 410 shown in FIG. 4. Adjustable sections 610 can be of any suitable size and shape.

#### RF Addressable Pressure Monitor

FIG. 7 is a schematic view of an RF addressable pressure monitor 700 in accordance with an embodiment presented herein. In some embodiments, RF addressable pressure monitor 700 is configured to be placed on a user and comprises a pressure sensor 710 operatively connected to an RFID device 715 disposed on a substrate 730. In some embodiments, pressure sensor 710 is a microelectromechanical system (MEMS) sensor on the order of 1 mm. The relatively small size of a MEMS pressure sensor allows easy placement on the user. Such MEMS sensors use a change in resistance, change in capacitance, change in voltage, or a piezoelectric effect to

6

convert changes in pressure on a sensing membrane to a voltage, current, or frequency change in the output signal.

Pressure sensor 710 is coupled to a wire 740 coupled to a radiofrequency (RF) device 715 on substrate 730, which can be in the form of a surface patch or bandage. Substrate 730 can include an adhesive material on one surface for affixing to the skin of the patient. Substrate 730 can further include multiple layers. In some embodiments, RF device 715 and RF antenna 760 can be integrated within layers of substrate 730.

In some embodiments, pressure sensor 710 could be an air or fluid filled contained volume coupled to an appropriate sensor through a tube communicating with the sensing membrane. The sensor could therefore be separate from the bandage packaging.

In some embodiments, RF device 715 comprises a RF antenna 760 and a battery 750 coupled to RFID chip 720 to provide power and to transmit data. RF device 715 powers pressure sensor 710, and interprets or relays the data from pressure sensor 710 to an interrogating reader. The RF device can be passive, pass-active (battery assisted), or fully active (battery dependent) depending upon the frequency of desired reads, the estimated distance of the interrogating device from the RF device, and the power consumption needs of the RF device. In alternative embodiments, the pressure sensor is integrated with Bluetooth, ZIGBEE or other radios compatible with wireless devices such as cell phones.

Substrate 730 (e.g., a layer of an adhesive bandage) is used to maintain RF device 715 and battery 750 on the surface of the user's skin or clothing. In some embodiments, sterile gauze can be placed between the electronic components and the surface of the skin.

In operation, a pressure change between pressure sensor 710 and the support surface is registered at pressure sensor 710. In the embodiment shown, the pressure data is then communicated to RF device 715 coupled to pressure sensor 710. In the embodiment shown, pressure sensor 710 and RF device 715 are powered by battery 750. Battery 750 can be substantially rigid or can be flexible. As would be appreciated by persons of skill in the art, RF device 715 and/or pressure sensor 710 can be powered by other techniques. Adhesive bandage material can be used to house and maintain RF device 715, battery 750, and pressure sensor 710. Additional external sensors can further be included in pressure monitor 700, e.g., in the adhesive bandage material or on substrate 730. Sterile gauze can be present in between adhesive bandage or substrate 730 and the surface of the user's skin or clothing.

FIG. 8 is a top view of a bandage 810 incorporating a pressure monitor 800 and substrate 830 in accordance with an embodiment presented herein. Similar to the pressure monitor shown, for example, in FIG. 7, pressure monitor 800 can comprise an RF device 815 and RF antenna 860. In the embodiment illustrated in FIG. 8, the RF device is placed on top of substrate 830. In FIG. 8 the bandage is an oval shape, of course the bandage could be any other suitable shape. Bandage 810 can be used with any of the pressure monitors described above.

FIG. 9 is a top view of a bandage 910 incorporating a pressure monitor 900 and substrate 930 in accordance with an embodiment presented herein. Similar to the pressure monitor shown, for example, in FIG. 7, pressure monitor 900 can comprise an RF device 915, RF antenna 960, and battery 950.

FIG. 10 is an RF device 1000 according to an embodiment. RF device 1000 is coupled to one or more external sensors 1010a-1010n. RF device 1000 includes RF core 1020, an analog to digital converter (ADC) 1030, and one or more antennas 1040. These components are mounted or formed on

a substrate. Additionally, the RF core **1020** and/or ADC **1030** can be included in an integrated circuit. RF device **1000** can also include one or more sensor elements **1050a-1050n**. Sensor elements **1050a-1050n** can be included in the integrated circuit, on the substrate, external to substrate, or in any combination of the above. Any compatible sensor element can be used as sensor element.

External sensors **1010a-1010n** include the sensors (e.g., MEMS sensor) described above for measuring compartment pressure. These external pressure sensors can be coupled to a pressure probe through a wire connector or an inelastic fluid filled tube. In an alternate embodiment, a fiber optic connection can be used.

Various types of sensor elements can be implemented as sensors **1050a-1050n** or external sensors **1010a-1010n**. For example, integrated or external sensor can include a temperature sensor element that generate information indicating ambient temperature; a pH sensor element; or other biological or chemical sensors. The system can include other types of sensor elements or combinations thereof, as would be apparent to persons skilled in the relevant art(s). Testing has shown that some RFID reader chips are not well suited to read complex RFID sensors due to timing and/or power issues. The readers are essentially meant to read ID numbers and have a very short interrogation/response cycle time. Furthermore when the technology is passive (as is the case for most RFID) substantial power fluctuations occur on the RFID chip and this affects sensor accuracy.

RFID core **1020** includes a communications module coupled to antenna **1040**, an RFID tag logic module, a power module and memory. In an embodiment, the memory stores an identifier for the RFID tag associated with the pressure sensor. The tag identifier, for example, may be used to associate the RF addressable sensor with an individual. In this example, a provider could maintain a database mapping tag identifiers to individuals.

A modified RFID chip can be used to facilitate these readers to read the pressure monitors comprising a complex MEMS sensor. Such a modified chip includes a serial peripheral interface (SPI) port and allows pre-processed sensor data to be stored in memory directly linked to the ID interrogation process of the RFID tag. This type of RFID tag therefore serves as a low cost "pass-through" radio. This design and method allows any sensor to be connected to common RFID technology and be read directly with current RFID enabled cell phones. The technology can be configured for ISO 15693 tags for example and is directly compatible with multiprotocol 13.56 MHz RFID reader chips for cell phones such as the PN 544 C2 reader chip made by NXP.

Different circuit designs and options are possible for the pass through method. FIG. **11** depicts an exemplary system **1100** having a modified RFID chip, and antenna **1190** according to an embodiment. FIG. **11** illustrates how complex sensors can be handled using a passive modified RFID radio, where the processed sensor data is passed through the RFID core as part of the standard interrogation-transmission of RFID data. The system **1100** includes a plurality of external sensors. In embodiments, the plurality of external sensors includes a complex calibrated external MEMS sensor **1110** and an ultra-precise external thermistor to allow medical grade combined pressure and temperature sensor measurements.

Each of the plurality of external sensors is coupled to a sensor interface **1120**. Sensor interface **1120** includes an analog to digital converter (ADC) and multiplexer **1130**, an external microprocessor (MCU) and firmware **1140**, and memory **1150**. Using an external microprocessor and firmware allows

compression of complex sensor data and extremely fast passage of information via the RFID chip, well within the limits of current standard RFID reader chips. Sensor interface **1120** further includes an external power source (e.g. battery, energy harvesting, solar, chemical, motion, etc.) that also can include a reference voltage calibration circuit. In an embodiment, sensor interface **1120** is included in a separate chip.

Sensor interface **1120** is coupled to modified RFID chip **1160**. The command set for the external MCU **1140** is passed through the RFID chip **1160**. The memory on the RFID chip is cleared either when full or bumped with each new interrogation or sensor data download or by external command from the RFID interrogator (e.g., a cell phone, or other wireless networkable device).

The RFID chip **1160** and sensor interface **1120** of FIG. **11** can be integrated into a single hybrid chip, whereby the packaged sensor data is placed in memory and where the main processor would be powered by the external power source and the communication part built to handle the constraints imposed by current RFID interrogators. Alternatively, the components of sensor interface **1120** can be included in a separate integrated circuit chip.

Various designs are possible for the fully integrated chip. The system of FIG. **11** illustrates the combination of an external temperature sensor **1170**, external MEMS sensor **1110**, and other sensor(s) **1180**. For temperature on chip a single calibration point digital sensor can be used. Such sensor technology is described in U.S. Pat. No. 7,461,972 that is included by reference in its entirety.

#### Network

FIG. **12** is a block diagram of an illustrative network for monitoring one or more pressure sensors integrated with RF devices and adjusting a support structure to accommodate for changes in pressure, in accordance with an embodiment of the present invention. The network includes one or more RF addressable sensors **1200**, one or more RFID/sensor readers **1250** and a controller **1260**. Exemplary RF addressable sensors are described above. The network may optionally include a communications network **1270** coupled to the controller **1260** and a remote monitoring station **1280**.

Communications network **1270** is a publicly accessible communications network. Communications network **1270** may be a wired network, wireless network, or a combination thereof. In another embodiment, communications network **1270** is a private network or a hybrid network including public and private portions. Persons skilled in the relevant art(s) will recognize that various network architectures could be used for communication network **1270**.

Wireless RFID/sensor reader **1250** includes logic to read sensor data and RFID tag data transmitted by RF addressable sensor **1200**. In an embodiment, wireless RFID/sensor reader **1250** also includes logic to process the received sensor data. Wireless RFID/sensor reader **1250** can be any wireless device capable of communicating via an air interface protocol with RF addressable sensor **1200**. In some embodiments, wireless RFID/sensor reader **1250** could be a wireless phone, a personal digital assistant (PDA), a computer having wireless communications capabilities, or other type of mobile, handheld, and/or computing device (e.g., an iPad).

According to an embodiment, signals are exchanged between the wireless RFID/sensor reader **1250** and RF addressable sensor **1200** according to one or more protocols. In an embodiment, reader **1250** and the RF addressable sensor **1200** communicate via a single protocol for both RFID tag communications and sensor communications. In an alternate

embodiment, reader **1250** and RF addressable sensor **1200** communicate via a first protocol for RFID tag communications and via a second protocol for sensor communications. Examples of protocols used for RFID tag communications include binary tree traversal, HF ISO 15693 and EPC global Gen 2. An embodiment is also applicable to any other types of communication protocols between tags and readers otherwise known or yet to be developed.

RFID/sensor reader **1250** is coupled to a controller **1260**. RFID/sensor reader **1250** communicates data obtained from the one or more RF addressable sensors **1200** to controller **1260**. Controller **1260** includes a pressure monitoring module **1264** and a support structure adjustment module **1266**.

Pressure monitoring module **1264** is configured to determine whether a pressure adjustment needs to be made to the support structure and isolates one or more cells to adjust. In an alternative embodiment, pressure monitoring module **1264** may be included as a component of RFID/sensor reader **1250** or distributed between the RFID/sensor reader and the controller **1260**. Pressure monitoring module **1264** communicates adjustment information to support structure adjustment module **1266**.

Support structure adjustment module **1266** is configured to adjust one or more cells in the support structure. In an embodiment, support structure adjustment module **1266** includes logic to determine the amount of adjustment to make to a specific cell. In an alternate embodiment, pressure monitoring module **1264** determines the amount of adjustment to make to a specific cell.

In an embodiment, controller **1260** and/or RFID/sensor reader **1264** communicates data to an external monitoring station. Controller **1260** and/or RFID/sensor reader **1250** may communicate all data obtained to external monitoring station **1280**. In addition or alternatively, controller **1260** and/or RFID/sensor reader **1250** may communicate only when certain conditions are detected. For example, controller **1260** and/or RFID/sensor reader **1250** may alert the external monitoring station **1280** when pressure in a certain area remains elevated and/or is not reduced after a series of adjustments.

External monitoring station **1280** receives sensor data over network **1270**, and processes the data. In an embodiment, the system associates tag identification data for an RF addressable sensor with an individual. External monitoring station **1280** may store data for each RF addressable sensors associated with an individual. The external monitoring station **1280** may analyze the pressure data associated with the individual and make an independent assessment of whether adjustments should be made to the support structure. External monitoring station **1280** may further be configured to communicate a request to adjust the structure to reduce pressure measurements for one or more tags associated with an individual. Records for individuals may be stored in a database **1282** coupled to external monitoring station **1280**.

In an embodiment, a healthcare provider determines if medical intervention is necessary based on alerts from RFID/sensor reader **1264**, controller **1266**, and/or external monitoring station **1280**. External monitoring station **1280** can display historical data or trends for one or more individuals.

#### Methods

FIG. **13** is a flowchart **1300** of a method for monitoring pressure and adjusting a support structure to compensate for measured pressure, according to embodiments of the present invention. Flowchart **1300** is described with reference to the embodiment of FIG. **12**. However, flowchart **1300** is not limited to that embodiment.

In step **1310**, pressure monitoring module **1264** obtains pressure data from one or more RF addressable sensors **1200** placed on an individual. The pressure monitoring module **1264** may also obtain a tag identification number associated with the RF addressable sensor **1200** providing sensor data. In an embodiment, RFID/sensor reader **1250** polls the one or more RF addressable sensors **1200**. In an alternate embodiment, the one or more RF addressable sensors **1200** are configured to periodically send data to RFID/sensor reader **1250**. RFID/sensor reader **1250** then communicates the received data to pressure monitoring module **1264**. In embodiments RFID/sensor reader **1250** may process the sensor data, e.g., to calibrate or smooth the received data, prior to communicating the data to pressure monitoring module **1264**.

In step **1320**, a determination is made whether the pressure data indicates an adjustment is required. In an embodiment, this determination is made on a per RF addressable sensor basis. For example, pressure monitoring module **1364** may determine for an RF addressable sensor whether the pressure data exceeds a threshold. In addition, or alternatively, the determination may be based on a historical trend for the RF addressable sensor. For example, if the pressure data has been consistently increasing over a predetermined period of time, an adjustment may be indicated for the RF addressable sensor. The networkable device, or associated computing system, can also compare the pressure data to the patient's diastolic blood pressure or other measurement, and calculate relevant clinical gradients in real time. As would be appreciated by persons of skill in the art, other techniques for determining whether an adjustment is required may be used with the present invention. If an adjustment is required, operation proceeds to step **1330**. If no adjustment is required, operation returns to step **1310**.

In step **1330**, one or more cells of the support structure to be adjusted are identified and adjusted. One method for identifying the cell or cells to adjust is discussed in FIG. **14**. As would be appreciated by persons of skill in the art, other techniques may be used in the present invention, e.g. triangulation of the sensors position by multiple RFID interrogators.

In step **1340**, pressure monitoring module **1264** obtains pressure data from the RF addressable sensors identified for adjustment. In an embodiment, pressure data may be obtained from all RF addressable sensors, as in step **1310**.

In step **1350**, a determination is made whether the pressure measurements in the RF addressable sensors identified for adjustment has improved. If pressure measurements indicate that the pressure data still indicates adjustment is necessary, pressure monitoring module may repeat step **1340** and **1350** over a pre-defined period of time after an initial adjustment is made. If improvement is not realized over that period of time, pressure monitoring module **1264** may repeat step **1330** to alter the adjustments. Additionally, if no improvement is achieved, the pressure monitoring module **1264** may alert external monitoring station **1280** of a potential bedsore/pressure sore risk.

If pressure measurements indicate an improvement, the adjustments made in step **1330** may be maintained for a specific period of time. After that time has expired, the system may return the cell or cells to their status prior to the adjustment.

FIG. **14** illustrates a flowchart **1400** for a method for determining an adjustment for one or more cells in a support structure, in accordance with embodiments of the present invention. FIG. **14** is described with reference to the embodiments of FIG. **12**. However, the method is not limited to that embodiment.

11

In step **1410**, the support structure is divided into one or more zones or clusters. FIG. **15A** depicts an exemplary support structure. As shown in FIG. **15A**, the support structure is divided into a plurality of zones **1520**. The zones may be of equal size and shape as shown in FIG. **15A**. Alternatively, the zones may be defined based on the likely position of an individual on the support structure, as depicted in FIG. **15B**. As would be appreciated by persons of skill in the art, other arrangements for zones could be used with the present invention.

In step **1420**, one or more zones may be further divided into a plurality of sub-zones. FIG. **15A** depicts a zone **1520** having a plurality of sub-zones. In embodiments, a sub-zone may be further divided into clusters. Step **1420** is optional.

In step **1430**, a first zone for adjustment is identified. In an embodiment, the pressure monitoring module **1264** prioritizes zones based on likelihood of a pressure injury occurring in the zone. For example, the zone associated with an individual's sacrum may be prioritized first.

In step **1440**, cells in the identified zone are adjusted. For example, the cells may be adjusted as described above in FIG. **3**.

In step **1445**, pressure data is obtained from RF addressable sensors identified for adjustment.

In step **1450**, a determination is made whether an improvement in pressure is reflected in the obtained data. If an improvement is indicated, operation proceeds to step **1460**. If no improvement is indicated by the data, operation proceeds to step **1452**.

Note that steps **1440** and **1450** may be repeated over a pre-determined period of time before an action is taken to give time for pressure changes to be reflected.

In step **1452**, a determination is made whether all zones in the support structure have been processed. If all zones have been processed, an alert may be sent to external monitoring station **1280** and processing of flowchart **1400** ends. If additional zones remain to be processed, operation proceeds to step **1454**.

In step **1454**, the next zone is identified. In embodiments, pressure monitoring module **1264** includes data specifying an order to process zones.

Operation then returns to step **1440**.

In step **1460** (if improvement is indicated in step **1450**), a sub-zone within the zone is identified. As with the zone, the pressure monitoring module **1264** may include data specifying an order to process sub-zones within a zone. Step **1460** is optional.

In step **1462**, cells in the sub-zone are adjusted. For example, the cells may be adjusted as described above in FIG. **3**.

In step **1464**, pressure data is obtained from RF addressable sensor identified for adjustment.

In step **1466**, a determination is made whether an improvement in pressure is reflected in the obtained data. If an improvement is indicated, operation proceeds to step **1470**. If no improvement is indicated by the data, operation proceeds to step **1490**.

Note that steps **1464** and **1466** may be repeated over a pre-determined period of time before an action is taken to give time for pressure changes to be reflected.

In step **1470**, a first cell within the sub-zone (or zone) is identified. As with the zone, the pressure monitoring module **1264** may include data specifying an order to process cells within a zone or sub-zone.

In step **1472**, the cell is adjusted. For example, the cell may be adjusted as described in FIG. **3**.

12

In step **1474**, pressure data is obtained from the RF addressable sensor identified for adjustment.

In step **1476**, a determination is made whether an improvement in pressure is reflected in the obtained data. If an improvement is indicated, operation proceeds to step **1478**. If no improvement is indicated by the data, operation proceeds to step **1480**.

Note that steps **1474** and **1476** may be repeated over a pre-determined period of time before an action is taken to give time for pressure changes to be reflected.

In step **1478**, a determination is made whether additional cells should be processed. If additional cells should be processed, operation proceeds to step **1480**. If no additional cells are to be processed, operation ends.

In step **1480**, a determination is made whether all cells in zone or sub-zone have been processed. If all cells have been processed, an alert may be sent to external monitoring station **1280** and processing of flowchart **1400** ends. If additional cells remain to be processed, operation proceeds to step **1482**.

In step **1482**, the next cell for adjustment is determined and operation returns to step **1472**.

In step **1490**, a determination is made whether all sub-zones in the support structure have been processed. If all sub-zones have been processed, an alert may be sent to external monitoring station **1280** and processing of flowchart **1400** ends. If additional sub-zones remain to be processed, operation proceeds to step **1494**.

In step **1494**, the next sub-zone is identified. In embodiments, pressure monitoring module **1264** includes data specifying an order to process zones.

Operation then returns to step **1462**.

#### Computer Architecture

FIG. **16** illustrates a block diagram of a data processing unit **1603** that can be used to implement portions of the RFID reader/sensor or controller illustrated in FIG. **12**. It is noted that the entities shown in FIG. **12** may be implemented using any number of data processing units **1603**, and the configuration actually used is implementation specific.

Data processing unit **1603** may represent a computer, a hand-held computer, a lap top computer, a personal digital assistant, a mobile phone, and/or any other type of data processing device. The type of data processing device used to implement the entities shown in FIG. **12** is implementation specific.

Data processing unit **1603** includes a communications medium **1610** (such as a bus, for example) to which other modules are attached.

Data processing unit **1603** also includes one or more processors **1620** and a main memory **1630**. Main memory **1630** may be RAM, ROM, or any other memory type, or combinations thereof.

Data processing unit **1603** may also include secondary storage devices **1640** such as but not limited to hard drives **1642** or computer program product interfaces **1644**. Computer program product interfaces **1644** are devices that access objects (such as information and/or software) stored in computer program products **1650**. Examples of computer program product interfaces **1644** include, but are not limited to, floppy drives, CD drives, DVD drives, ZIP drives, JAZ drives, optical storage devices, universal serial bus (USB), etc. Examples of computer program products **1650** include, but are not limited to, floppy disks, CDs, DVDs, ZIP and JAZ disks, memory sticks, memory cards, or any other medium on which objects may be stored.

13

The computer program products **1650** include a computer useable medium **1652** on which objects may be stored, such as but not limited to optical mediums, magnetic mediums, etc.

Control logic or software may be stored in main memory **1630**, second storage device(s) **1640**, and/or computer program products **1650**.

More generally, the term “computer program product” refers to any device in which control logic (software) is stored, so in this context a computer program product could be any memory device having control logic stored therein. The invention is directed to computer program products having stored therein software that enables a computer/processor to perform functions of the invention as described herein.

The data processing unit **1603** may also include an interface **1660** which may receive objects (such as data, applications, software, images, etc.) from external entities **1680** via any communications media including wired and wireless communications media. In such cases, objects **1670** are transported between external entities **1680** and interface **1660** via signals **1665**, **1675**. In other words, signals **1665**, **1675** include or represent control logic for enabling a processor or computer to perform the functions of the invention. According to embodiments of the invention, such signals **1665**, **1675** are also considered to be computer program products, and the invention is directed to such computer program products.

#### CONCLUSION

While various embodiments of the present invention have been described above, it should be understood that they have been presented by way of example only, and not limitation. It will be apparent to persons skilled in the relevant art that various changes in form and detail can be made therein without departing from the spirit and scope of the invention. Thus, the breadth and scope of the present invention should not be limited by any of the above-described exemplary embodiments, but should be defined only in accordance with the following claims and their equivalents.

What is claimed is:

**1.** A method for monitoring pressure at one or more points on an individual and automatically adjusting one or more sections of a support structure having a plurality of adjustable cells, wherein the support structure is divided into a plurality of zones and one or more of the zones is divided into a plurality of subzone, the method comprising:

periodically receiving with one or more processors, localized contact pressure data from one or more radio frequency (RF) addressable sensors placed on an individual;

determining whether an adjustment in the support structure is required using the received localized contact pressure data

when an adjustment is required, systematically adjusting cells located within the plurality of zones, one zone at a time, until a required change in localized pressure data is indicated;

if the required change in localized pressure data is indicated for a zone, systematically adjusting cells within, the plurality of subzones for that zone, one subzone at a time, until the required change in localized pressure data is indicated; and

if the required change in localized pressure data is indicated for a subzone, systematically adjusting cells in that subzone, one cell at a time, until the required change in localized pressure data is indicated.

14

**2.** The method of claim **1**, further comprising receiving a tag identification number for each of the one or more RF addressable sensors.

**3.** The method of claim **1**, wherein receiving localized contact pressure data from one or more RF addressable sensors includes polling the RF addressable sensors.

**4.** The method of claim **1**, wherein determining whether an adjustment is required includes determining whether the received localized contact pressure data from one or more of the RF addressable sensors exceeds a threshold.

**5.** The method of claim **1**, wherein determining whether an adjustment is required is based on a historical trend for one or more of the RF addressable sensors.

**6.** The method of claim **5**, wherein the historical trend includes information indicating that the received localized contact pressure data has increased over a predetermined period of time.

**7.** The method of claim **1**, wherein an order for systematically adjusting one or more zones is based on the likely position of the individual on the support structure.

**8.** The method of claim **1**, wherein an order for systematically adjusting one or more zones is based on the likelihood or severity of a pressure injury occurring in the zone.

**9.** The method of claim **1**, wherein determining whether an adjustment in the support structure is required is based on whether the received localized contact pressure data is below a threshold pressure.

**10.** The method of claim **1**, further comprising sending an alert to an external monitoring station if the required change in the pressure data is not indicated after the adjustments are completed.

**11.** The method of claim **1**, further comprising: maintaining the adjustments for a predetermined period of time; and receiving updated localized contact pressure data from the one or more RF addressable sensors.

**12.** The method of claim **11**, further comprising: returning one or more of the adjustable sections to a pre-adjusted level following the predetermined period of time.

**13.** The method of claim **1**, wherein adjusting one or more identified sections includes inflating one or more of the identified sections.

**14.** The method of claim **1**, wherein adjusting one or more identified sections includes deflating one or more of the identified sections.

**15.** A system for preventing and/or treating pressure wounds on an individual, the system comprising:

a support structure including a plurality of adjustable cells, wherein the support structure is divided into a plurality of zones and one or more of the zones is divided into a plurality of subzones;

an RFID sensor reader configured to receive localized contact pressure data from one or more RF addressable sensors placed adjacent to the skin of the individual;

a processor coupled to the support structure and the RFID sensor reader, wherein the processor is configured to:

determine whether the localized contact pressure data in an RF addressable sensor in the one or more RF addressable sensors exceeds a predetermined threshold, and isolate a location on the individual of the RF addressable sensor by systematically adjusting the adjustable cells in the plurality of zones, one zone at a time until a required change in the localized contact pressure data is indicated for a zone and adjusting the adjustable cells in the plu-

**15**

ality of subzones for that zone, one subzone at a time, until the required change in the localized contact pressure data is indicated.

**16.** The system of claim **15**, further comprising an actuator coupled to the processor and the one or more adjustable cells.

**17.** The system of claim **16**, further comprising a hose assembly connected to the one or more adjustable sections, the hose assembly comprising:

- a means of introducing pressure;
- a central line operatively connected to the means of introducing pressure; and
- one or more branch lines operatively connected to the central line and operatively connected to the one or more adjustable sections,

wherein the hose assembly is configured to adjust the one or more identified sections.

**18.** The system of claim **17**, wherein the hose assembly is configured to adjust the one or more identified sections with air pressure.

**16**

**19.** The system of claim **17**, wherein the hose assembly is configured to adjust the one or more identified sections with fluid pressure.

**20.** The system of claim **15**, wherein the RF addressable sensor is included in a bandage affixed to the skin of the individual.

**21.** The system of claim **15**, wherein the support structure is a bed.

**22.** The system of claim **15**, wherein the support structure is a pad configured for use on a bed.

**23.** The system of claim **15**, wherein the support structure is a chair.

**24.** The system of claim **15**, wherein the support structure is a wheel chair.

**25.** The system of claim **15**, wherein the support structure is a pad configured for use on a chair.

\* \* \* \* \*